



Advancements in Deep Learning Techniques for Enhanced Assessment of Fetal Anomalies in Prenatal Imaging: Review of Current Applications and Future Directions

¹-Bandr Abdullah Mohammed Al Jaloud,²-Hussain Mohammed Khalawialruwily,³-Atiah Abdularazqabdullah Mohammed,⁴-Hesahsayaf Al_Mohemed,⁵-Mohammed Abdulrahman Obaid Alrowais,⁶-Bassam Ali Tumayhi,⁷-Mohammad Qassim Ahmad Hijri,⁸-Khalid Ahmed Ali Maghfuri,⁹-Hani Hossen Aseeri,¹⁰- Mohammed Mnawer H Alrowaili,¹¹- Fahad Muteb Jaber Aljaber,¹²-Mohammed Obaid Alharbi,¹³- Abdulrahman Dhafi Sair Alanazi,¹⁴-Sami Mohammed Saleh Alamri

1. KSA, Ministry Of Health, Samira General Hospital
2. KSA, Ministry OfHealth, King Salman Hospital
3. KSA, Ministry OfHealth, King Fahad Hospital Jazan
4. KSA, Ministry OfHealth, Al_MiqatgeneralHospital
5. KSA, Ministry OfHealth, Diriyah Hospital
6. KSA, Ministry OfHealth, PRINCE MOHAMMED BIN NASSER HOSPITAL- JAZAN
7. KSA, Ministry OfHealth, Prince Mohammad Bin Nasser Hospital At Jazan
8. □KSA, Ministry OfHealth, King Fahd Central Hospital Jazan
9. KSA, Ministry OfHealth
10. KSA, Ministry OfHealth, Swyer General Hospital
11. KSA, Ministry OfHealth, Swyer General Hospital
12. KSA, Ministry OfHealth, MiqatGeneral Hospital MOH
13. KSA, Ministry OfHealth, Al Hamra Primary Health Care Center
14. KSA, Ministry OfHealth, Tabuk Health ClusterKing Fahad Multi-Specialty Hospital

Abstract

Background: Deep learning (DL) has emerged as a transformative technology in the field of medical imaging, particularly in prenatal assessments. The application of DL algorithms in fetal imaging aims to address challenges such as human subjectivity and interobserver variability, while enhancing diagnostic accuracy.

Methods: This review synthesizes recent advancements in the application of deep learning techniques for evaluating fetal anomalies. A comprehensive literature search was conducted to gather evidence on the efficacy of DL in various aspects of prenatal imaging, including anatomical assessment, biometric measurements, and the detection of congenital abnormalities.

Results: The findings indicate that deep learning models exhibit superior performance in identifying normal and abnormal fetal anatomy compared to traditional methods. These models effectively classify images, localize anatomical structures, and segment key features, significantly reducing examination times and improving workflow. Furthermore, multiple studies demonstrate that DL can mitigate the impact of human error, achieving classifications that rival or exceed those of experienced sonographers.

Conclusion: The integration of deep learning into prenatal imaging holds considerable promise for enhancing diagnostic capabilities and improving patient outcomes. As these technologies evolve, they offer the potential to support clinicians, particularly in resource-limited settings where access to skilled sonographers is limited. Future research should focus on refining these models and ensuring their clinical applicability to maximize the benefits of deep learning in obstetric care.

Keywords: Deep Learning, Fetal Imaging, Prenatal Assessment, Congenital Anomalies, Ultrasound Technology

Received: 07 October 2023

Revised: 22 November 2023

Accepted: 06 December 2023

1. Introduction

Deep learning (DL) is regarded as the preeminent artificial intelligence (AI) instrument for image analysis overall [1,2]. Deep learning algorithms excel in picture identification and classification, making them helpful in medical imaging. Deep learning models have shown the capacity to equal or surpass human performance in tasks like image categorization, detection, and segmentation [3-5]. Consequently, deep learning has been suggested as a prospective auxiliary instrument for physicians in medical imaging. A recent assessment determined that more than 80% of published research on the use of AI in medical imaging employed a deep learning technique [1,2,6].

In recent years, deep learning has garnered significant appeal in the domain of prenatal imaging, as seen by the substantial volume of published scientific research using this methodology [7-10]. In fetal imaging, deep learning (DL) is anticipated to mitigate issues associated with human analysis, such as subjectivity and interobserver variability, while also decreasing examination durations. Additionally, it may be used in the instruction of novice and unskilled physicians [11-13]. This State-of-the-Art Review offers a thorough examination of the use of deep learning in prenatal imaging. We elucidate the use of deep learning in prenatal imaging, emphasizing the evaluation of normal and abnormal fetal anatomy, biometric measures, and intrapartum ultrasonography.

Deep learning

'Artificial intelligence' refers to a computer's capacity to execute activities linked to human intellect, including learning, decision-making, visual perception, and voice recognition. Unlike human thinking, AI algorithms are proficient at detecting intricate patterns in data to provide an automated quantitative answer to a problem [1]. This indicates that their outcomes are more precise and repeatable than those of people. Machine learning algorithms, a subset of artificial intelligence, empower computers to learn and improve their performance via 'experience' (utilizing available data), without explicit programming. Numerous machine-learning techniques exist, with deep learning (DL) being the most significant in the domain of medical imaging (Figure 1) [2].

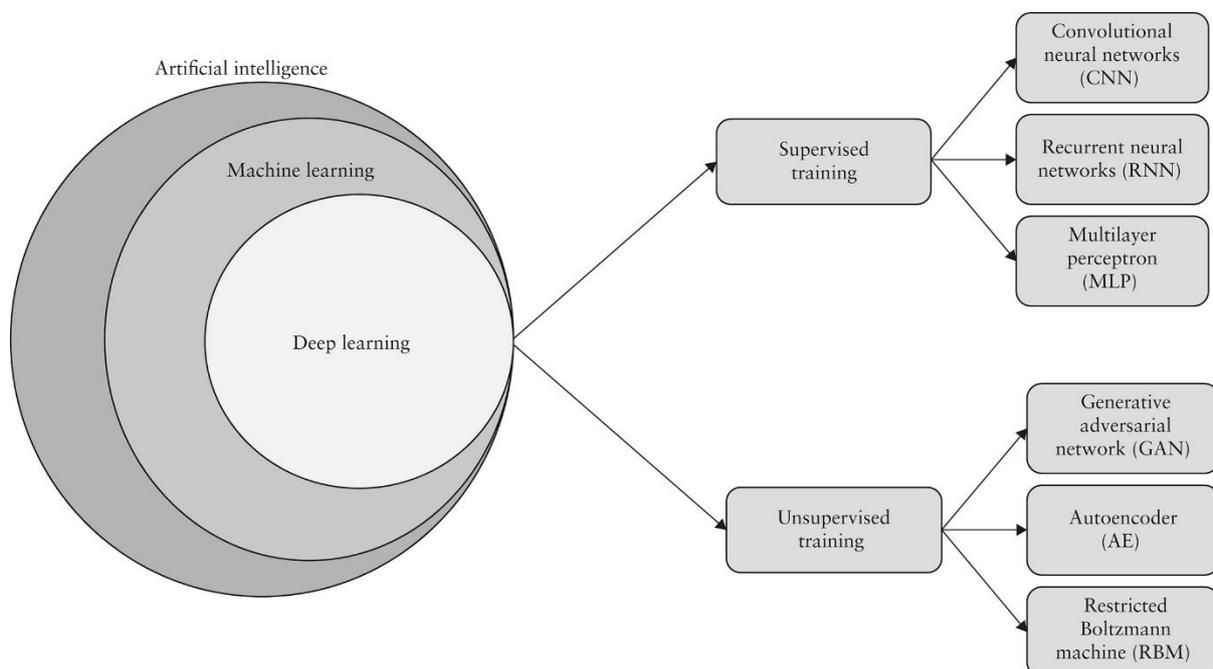


Figure 1. Summary of primary categories of deep learning algorithms categorized by training methodologies.

The architecture of deep learning models is complex and comprises several deep layers of artificial neural networks. Convolutional neural networks (CNN) are the most often used, however several other forms of deep neural networks exist (Figure 1). Deep learning models may examine extensive datasets in a layered, non-linear fashion, using pattern recognition to extract highly representative picture attributes for the purpose of labeling an image (e.g., as normal or abnormal). [14] Deep learning models may be constructed with either a supervised or unsupervised learning methodology. A supervised deep learning model, the most prevalent form, necessitates tagged or 'ground-truth' data as input for the neural networks during the training phase. The model's performance is then evaluated using unlabeled data, including normal brain scans and images exhibiting ventriculomegaly that have not been annotated by human operators, during the testing phase. Thereafter, the deep learning model will provide a forecast and categorize the picture. Conversely, unsupervised learning methods do not need labels. The deep learning model identifies primary patterns and similarities in the input data to categorize the photos in the output [15].

2. The Advantages of Utilizing Deep Learning In Fetal Imaging

Prenatal ultrasonography has significantly advanced over the years; nonetheless, the overall detection rates of congenital abnormalities continue to be low [16]. A primary reason for this is the human aspect. Navigating the ultrasound probe through intricate fetal anatomy to achieve the appropriate scanning plane, evaluating each fetal anatomical feature, and arriving at an accurate diagnosis requires years of training and comprehensive understanding of fetal anatomy [17-20]. Furthermore, issues intrinsic to ultrasonography, such as acoustic shadows, speckle noise, motion blurring, and indistinct boundaries, may potentially exacerbate the poor detection rates [21]. A further drawback of ultrasonography is the significant intra- and interobserver variability, particularly in biometric measures, which may lead to considerable inaccuracies in fetal weight estimate, leading in the misclassification of small- or large-for-gestational age fetuses [22].

3. The Mechanisms of Deep Learning In Fetal Imaging

The prospective applications of deep learning in obstetrics include the detection of normal and abnormal fetal anatomy as well as the assessment of fetal biometry. For these applications, deep learning models include one or a combination of up to four tasks: classification, localization, object identification, and segmentation, depending upon the required output. Classification designates a binary 'class label' to a picture, such as normal/abnormal or correct/incorrect anatomical orientation. Localization determines the exact position of an item inside an image, facilitating the identification of anatomical landmarks and enabling automated measurements. Object detection integrates classification and localization, simultaneously identifying the position of fetal structures in a picture (and, if required, their measurement) while categorizing them as normal or abnormal. Ultimately, segmentation refers to the identification of an item inside the picture. It resembles localization, however, also evaluates the morphology (form, volume, and contour) of the item, and may be integrated with classification tasks to categorize the picture as normal or aberrant [5].

This innovative technology has characteristics that may assist both novice and seasoned operators. The automated assessment of biometric parameters or identification of anatomical landmarks would assist the novice operator conducting a fetal screening scan, while deep learning models designed to detect fetal malformations could bolster the confidence of the junior examiner in diagnosis and notify a more seasoned operator of subtle anomalies that might otherwise be missed [23,24].

4. The Potential of Deep Learning to Enhance Fetal Imaging

Biometric measures are used to assess gestational age (GA) and track fetal development. To do this, many fetal components, including the fetal head, abdomen, femur, cerebellum, and crown-rump length (CRL) (before to 14 weeks of gestation), are assessed using conventional biometry planes [25-27]. The

measurements are labor-intensive and dependent on the operator, necessitating accurate capture of the standard plane prior to the manual positioning of the calipers. Complete automation using deep learning may mitigate interobserver variability and decrease examination durations, hence enhancing workflow. This method may ultimately reduce tiredness and alleviate occupational injuries [28-30].

Various deep learning models have been created using diverse methodologies for the automated assessment of fetal head biometry (head circumference, occipitofrontal diameter, and biparietal diameter) and femur length [31-33]. The automatic measurement of fetal abdominal circumference presents more challenges owing to its uneven morphology and indistinct borders. Consequently, researchers have suggested using object identification or segmentation of fetal abdominal anatomical landmarks (stomach bubble, umbilical vein, fetal spine) before measuring the abdominal circumference [34-38]. Recent advancements in artificial intelligence have enabled researchers to create multitasking deep learning models that use segmentation to automatically conduct all biometric measures in the three conventional fetal planes. This strategy allows the DL algorithm to concurrently estimate the GA and GA [39, 40].

The assessment of crown-rump length (CRL) and nuchal translucency (NT) is a crucial component of the prenatal ultrasonography evaluation during the first trimester of gestation [41]. Automatic measurement of CRL and NT via deep learning models has been facilitated by 3D imaging and segmentation methodologies [42-44]. The benefit of using 3D ultrasound is that the deep learning model can identify and choose the optimal planes for conducting biometric measurements of the fetal head, belly, and femur.

For decades, ultrasonography has served as the primary imaging technique for diagnosing prenatal abnormalities. The standard procedure for prenatal ultrasound in evaluating fetal anatomy entails: first, accurate acquisition of standard fetal planes; second, identification and measurement of fetal anatomical structures; and third, categorization of the identified structures as normal or abnormal. Human operators take years of expertise to completely grasp this technique [45]. Conversely, deep learning algorithms may be taught in a very little period using substantial datasets, achieving performance comparable to or superior to that of human operators.

The International Society of Ultrasound in Obstetrics and Gynecology (ISUOG) has recommended many fetal standard planes to standardize the precise acquisition of these planes and minimize intra- and interobserver variability. A comprehensive assessment of fetal anatomy is an arduous and time-intensive endeavor. Deep learning algorithms may be taught to reliably detect several fetal standard planes, and multiple deep learning models have been built to automatically identify the primary fetal standard planes, including the brain, heart, face, and belly. In identifying fetal standard planes, deep learning models that execute object detection and segmentation tasks demonstrate greater accuracy than classification models, as they localize fetal anatomical landmarks prior to classifying the plane, akin to human methodology. Burgos-Artizzu et al. [46] conducted a comparison of 19 deep learning algorithms concerning the accurate identification of four anatomical standard planes (abdomen, brain, femur, and thorax) and discovered that the performance of the top models was comparable to that of a fully trained sonographer, while achieving a classification speed 25 times greater [47-50].

In the second phase, precise identification of normal fetal anatomy is essential to rule out congenital abnormalities. Deep learning algorithms can identify and annotate fetal anatomical components across several standard planes using object recognition and segmentation tasks. Manual structural segmentation is a tedious endeavor, characterized by significant intra- and interobserver heterogeneity. Segmentation deep learning algorithms have shown superior performance compared to both people and other AI models for this task [51].

5. The central nervous system (CNS) of the fetus

The fetal brain is among the most intricate fetal structures, and its examination during the second trimester necessitates the acquisition and assessment of many standard brain planes. Furthermore, the fetal brain experiences significant changes in structure and morphology throughout pregnancy, complicating its evaluation. Multiple deep learning models have been created for the automated detection

of standard planes in the embryonic brain and have shown effective performance [52-55]. Deep learning models can accurately recognize several brain anatomical features, including the lateral ventricles, choroid plexus, cavum septi pellucidi, thalami, cerebellum, cisterna magna, Sylvian fissure, and brainstem. Furthermore, deep learning models may be taught to execute automated assessments of fetal brain regions, including the lateral ventricles and cavum septi pellucidi. Another use of deep learning models in brain examination is the evaluation of embryonic cortical development. Deep learning algorithms may evaluate the morphology of cortical structures to predict the associated gestational age; if this gestational age does not align with the actual gestational age, the operator will be notified of a potential cortical developmental defect [56].

Central nervous system (CNS) malformations are among the most common congenital abnormalities. Nevertheless, some CNS abnormalities may not result in significant structural alterations and may remain undiagnosed during prenatal ultrasonography assessments [57,58]. Deep learning might serve as a diagnostic assistance instrument to enhance the detection rates of prenatal brain malformations and assist in the decision-making process. Deep learning models may be taught to identify structural anomalies in the fetal brain or spine on conventional screening planes and notify the operator of the existence and location of potential malformations. Furthermore, deep learning models may categorize the specific kind of abnormality (e.g., ventriculomegaly, intraventricular cyst, non-visualization of cavum septi pellucidi) seen in the fetal picture [59]. Lin et al. [60] revealed the development of a deep learning system capable of localizing and classifying nine distinct brain abnormalities using routine screening planes, with an overall accuracy of 99%.

Accurate evaluation of embryonic heart architecture necessitates the examination of many fetal anatomical landmarks and cardiac structures in well-defined standard planes. Fetal standard cardiac planes, including the four-chamber view, left ventricular outflow tract, right ventricular outflow tract, and three-vessel-and-trachea views, may be automatically obtained via deep learning models [61]. Fetal cardiac structures may be seen using deep learning algorithms that execute object identification or segmentation tasks. Current deep learning models can identify the four distinct chambers of the embryonic heart, as well as the foramen ovale, mitral and tricuspid valves, aorta, apex cordis, moderator band, left and right ventricular walls, interventricular septum, and pulmonary veins [62,63]. DL models could ascertain whether the picture corresponds to the end-systolic or end-diastolic phase of the fetal cardiac cycle based on the opening or closure of the atrioventricular valves. Segmentation deep learning algorithms facilitate the assessment of cardiac morphology by enabling automated quantification of fetal cardiac features, including the dimensions of the fetal heart chambers. It is crucial to note that, in several fetal diseases, including fetal growth restriction, cardiac shape may serve as a marker of pathology [64]. Deep learning models may also be used in the Doppler assessment of the fetal heart, as suggested by Sulas et al. [65]. The authors created a model capable of automatically evaluating pulsed-wave Doppler traces of left ventricular inflows and outflows, identifying early and late diastole and systole. Ultimately, deep learning algorithms may provide biometric heart metrics, including the cardiothoracic ratio and the cardiac axis angle [66,67].

Congenital heart disease (CHD) is the most prevalent birth abnormality and is linked to elevated infant death rates. The prenatal detection of congenital heart disease facilitates early planning and therapy of the problem, hence enhancing perinatal outcomes. Detection rates, however, exhibit significant variability mostly attributable to disparities in operator experience. The use of deep learning models may enhance prenatal identification rates of congenital heart disease by offering an objective and operator-independent evaluation of fetal cardiac pictures. Certain writers have suggested using deep learning models to notify the operator when a cardiac anomaly is observed. Nonetheless, there is a need for deep learning models that can recognize and classify numerous congenital heart defects in the field. As of now, deep learning models capable of identifying hypoplastic left heart syndrome and ventricular septal abnormalities have been developed via object detection or segmentation techniques. Concerning ventricular septal abnormalities, segmentation deep learning algorithms can accurately identify and

isolate the whole defect on the fetal heart septum, enabling precise determination of its dimensions [68-70].

The routine assessment of the placenta often includes ascertaining its position and echogenicity, as well as identifying characteristics indicative of aberrant invasive placentation. Placental biometry, associated with fetal smallness, pre-eclampsia, and other negative pregnancy outcomes, is not frequently conducted due to its time-consuming and operator-dependent nature. An entirely automated deep learning model might execute this work swiftly and consistently, therefore reducing interobserver variability, perhaps becoming placental biometry a valuable imaging biomarker [71]. Furthermore, these algorithms may evaluate the placenta's placement (anterior or posterior) and appearance (normal or pathological). Segmentation deep learning methods used with 3D ultrasonography may provide supplementary insights about the anatomy and volume of the placenta [72].

Placental lacunae are hypoechoic cavities located inside the placenta. While prevalent in most pregnancies, extensive, many, and/or irregular placental lacunae may indicate aberrant placental invasion. Abnormal invasive placentation is an obstetric disorder linked to increased maternal morbidity and death. Segmentation deep learning algorithms can effectively identify and localize placental lacunae with high accuracy [73].

A comprehensive prenatal ultrasound examination includes the evaluation of other fetal structures in addition to the brain, heart, and placenta. The use of deep learning (DL) is progressively broadening, with DL algorithms capable of identifying various fetal tissues, including the face, spine, kidneys, lungs, fat tissue, and sexual organs. Certain ultrasound manufacturers have begun including checklists of requisite standard planes and fetal anatomical components into the software of ultrasound machines, to assist and direct the operator throughout the examination [74,75].

6. Deep learning and ultrasonography during childbirth

Ultrasound is being used in the labor ward, proving effective in evaluating fetal head station, degree of bending, and position. Obtaining the accurate picture and doing the requisite measurements may need many minutes, in a context where delays in decision-making might lead to detrimental consequences. The deployment of a deep learning model capable of concurrently evaluating the station, angle, and position of the fetal head may contribute to routine labor ward operations. Research efforts have so far focused on creating deep learning models to evaluate the fetal occiput position during the second stage of labor, classifying it as occiput anterior, posterior, or transverse [76,77].

7. Conclusion

The eventual integration of deep learning in obstetrics and fetal imaging seems unavoidable. Deep learning has several benefits, including objectivity, repeatability, rapidity, and precision, with significant promise as an auxiliary instrument for prenatal ultrasonography. It is essential to recognize that these novel procedures are designed not to supplant specialists in the field, but to assist them and enhance workflow, so conserving time for both patients and clinicians. Furthermore, this technique may enhance healthcare in rural regions or low-income nations, where experienced sonographers are few and patients must traverse considerable distances for consultations. A considerable journey remains before deep learning may be completely integrated into therapeutic practice. Nevertheless, since the volume of papers in the subject increases annually, this may be realized sooner than anticipated.

References

1. Drukker L, Noble JA, Papageorghiou AT. Introduction to artificial intelligence in ultrasound imaging in obstetrics and gynecology. *Ultrasound Obstet Gynecol* 2020; 56: 498–505.
2. Litjens G, Kooi T, Bejnordi BE, Setio AAA, Ciampi F, Ghafoorian M, van der Laak JAWM, van Ginneken B, Sánchez CI. A survey on deep learning in medical image analysis. *Med Image Anal* 2017; 42: 60–88.
3. Hinton G. Deep Learning—A Technology With the Potential to Transform Health Care. *JAMA* 2018; 320: 1101.

4. Liu X, Faes L, Kale AU, Wagner SK, Fu DJ, Bruynseels A, Mahendiran T, Moraes G, Shamdas M, Kern C, Ledsam JR, Schmid MK, Balaskas K, Topol EJ, Bachmann LM, Keane PA, Denniston AK. A comparison of deep learning performance against health-care professionals in detecting diseases from medical imaging: a systematic review and meta-analysis. *Lancet Digit Heal* 2019; 1: e271–e297.
5. Fiorentino MC, Villani FP, Di Cosmo M, Frontoni E, Moccia S. A Review on Deep-Learning Algorithms for Fetal Ultrasound-Image Analysis. *Med Image Anal* 2023; 83: 102629.
6. Liu S, Wang Y, Yang X, Lei B, Liu L, Li SX, Ni D, Wang T. Deep Learning in Medical Ultrasound Analysis: A Review. *Engineering* 2019; 5: 261–275.
7. He F, Wang Y, Xiu Y, Zhang Y, Chen L. Artificial Intelligence in Prenatal Ultrasound Diagnosis. *Front Med (Lausanne)* 2021; 8: 729978.
8. Espinoza J, Good S, Russell E, Lee W. Does the Use of Automated Fetal Biometry Improve Clinical Work Flow Efficiency? *J Ultrasound Med* 2013; 32: 847–850.
9. Yazdi B, Zanker P, Wagner P, Sonek J, Pintoffl K, Hoopmann M, Kagan KO. Optimal caliper placement: manual vs automated methods. *Ultrasound Obstet Gynecol* 2014; 43: 170–175.
10. Matthew J, Skelton E, Day TG, Zimmer VA, Gomez A, Wheeler G, Toussaint N, Liu T, Budd S, Lloyd K, Wright R, Deng S, Ghavami N, Sinclair M, Meng Q, Kainz B, Schnabel JA, Rueckert D, Razavi R, Simpson J, Hajnal J. Exploring a new paradigm for the fetal anomaly ultrasound scan: Artificial intelligence in real time. *Prenat Diagn* 2022; 42: 49–59.
11. Zhang L, Portenier T, Paulus C, Goksel O. Deep Image Translation for Enhancing Simulated Ultrasound Images. *Medical Ultrasound, and Preterm, Perinatal and Paediatric Image Analysis. ASMUS 2020, PIPPI 2020. Lecture Notes in Computer Science, vol 12437. Springer: Cham, 2020; 85–94.*
12. Zhao C, Droste R, Drukker L, Papageorghiou AT, Noble JA. Visual-Assisted Probe Movement Guidance for Obstetric Ultrasound Scanning Using Landmark Retrieval. *Med Image Comput Comput Assist Interv* 2021; 12908: 670–679.
13. Sakai A, Komatsu M, Komatsu R, Matsuoka R, Yasutomi S, Dozen A, Shozu K, Arakaki T, Machino H, Asada K, Kaneko S, Sekizawa A, Hamamoto R. Medical Professional Enhancement Using Explainable Artificial Intelligence in Fetal Cardiac Ultrasound Screening. *Biomedicines* 2022; 10: 551.
14. Shazly SA, Trabuco EC, Ngufor CG, Famuyide AO. Introduction to Machine Learning in Obstetrics and Gynecology. *Obstet Gynecol* 2022; 139: 669–679.
15. Bakker MK, Bergman JEH, Krikov S, Amar E, Cocchi G, Cragan J, de Walle HEK, Gatt M, Groisman B, Liu S, Nembhard WN, Pierini A, Rissmann A, Chidambarathanu S, Sipek A, Szabova E, Tagliabue G, Tucker D, Mastroiacovo P, Botto LD. Prenatal diagnosis and prevalence of critical congenital heart defects: an international retrospective cohort study. *BMJ Open* 2019; 9: e028139.
16. van Nesselrooij AEL, Teunissen AKK, Clur SA, Rozendaal L, Pajkrt E, Linskens IH, Rammeloo L, van Lith JMM, Blom NA, Haak MC. Why are congenital heart defects being missed? *Ultrasound Obstet Gynecol* 2020; 55: 747–757.
17. Pinto NM, Keenan HT, Minich LL, Puchalski MD, Heywood M, Botto LD. Barriers to prenatal detection of congenital heart disease: a population-based study. *Ultrasound Obstet Gynecol* 2012; 40: 418–425.
18. Fadda GM, Capobianco G, Balata A, Litta P, Ambrosini G, D'Antona D, Cosmi E, Dessole S. Routine second trimester ultrasound screening for prenatal detection of fetal malformations in Sassari University Hospital, Italy: 23 years of experience in 42,256 pregnancies. *Eur J Obstet Gynecol Reprod Biol* 2009; 144: 110–114.
19. Rydberg C, Tunón K. Detection of fetal abnormalities by second-trimester ultrasound screening in a non-selected population. *Acta Obstet Gynecol Scand* 2017; 96: 176–182.
20. Pramanik M, Gupta M, Krishnan KB. Enhancing reproducibility of ultrasonic measurements by new users, CK Abbey, CR Mello-Thoms (eds). *SPIE Proceedings, vol 8673. Medical Imaging 2013: Image Perception, Observer Performance, and Technology Assessment, 2013; 6730Q.*
21. Meng L, Zhao D, Yang Z, Wang B. Automatic display of fetal brain planes and automatic measurements of fetal brain parameters by transabdominal three-dimensional ultrasound. *J Clin Ultrasound* 2020; 48: 82–88.

22. Sarris I, Ioannou C, Chamberlain P, Ohuma E, Roseman F, Hoch L, Altman DG, Papageorgiou AT, International Fetal and Newborn Growth Consortium for the 21st Century (INTERGROWTH-21st). Intra- and interobserver variability in fetal ultrasound measurements. *Ultrasound Obstet Gynecol* 2012; 39: 266–273.
23. Wright D, Wright A, Smith E, Nicolaides KH. Impact of biometric measurement error on identification of small- and large-for-gestational-age fetuses. *Ultrasound Obstet Gynecol* 2020; 55: 170–176.
24. Drukker L. Real-time identification of fetal anomalies on ultrasound using artificial intelligence: what's next? *Ultrasound Obstet Gynecol* 2022; 59: 285–287.
25. Salomon LJ, Alfrevic Z, Da Silva Costa F, Deter RL, Figueras F, Ghi T, Glanc P, Khalil A, Lee W, Napolitano R, Papageorgiou A, Sotiriadis A, Stirnemann J, Toi A, Yeo G. ISUOG Practice Guidelines: ultrasound assessment of fetal biometry and growth. *Ultrasound Obstet Gynecol* 2019; 53: 715–723.
26. Hadlock FP, Harrist RB, Carpenter RJ, Deter RL, Park SK. Sonographic estimation of fetal weight. The value of femur length in addition to head and abdomen measurements. *Radiology* 1984; 150: 535–540.
27. Snijders RJM, Nicolaides KH. Fetal biometry at 14–40 weeks' gestation. *Ultrasound Obstet Gynecol* 1994; 4: 34–48.
28. Industry Standards for the Prevention of Work Related Musculoskeletal Disorders in Sonography. *J Diagnostic Med Sonogr* 2017; 33: 370–391.
29. Gibbs V, Young P. A study of the experiences of participants following attendance at a workshop on methods to prevent or reduce work-related musculoskeletal disorders amongst sonographers. *Radiography* 2011; 17: 223–229.
30. Sinclair M, Baumgartner CF, Matthew J, Bai W, Martinez JC, Li Y, Smith S, Knight CL, Kainz B, Hajnal J, King AP, Rueckert D. Human-level Performance On Automatic Head Biometrics In Fetal Ultrasound Using Fully Convolutional Neural Networks. 40th Annual International Conference of the IEEE Engineering in Medicine and Biology Society (EMBC), 2018; 714–717.
31. Li P, Zhao H, Liu P, Cao F. Automated measurement network for accurate segmentation and parameter modification in fetal head ultrasound images. *Med Biol Eng Comput* 2020; 58: 2879–2892.
32. Rasheed K, Junejo F, Malik A, Saqib M. Automated Fetal Head Classification and Segmentation Using Ultrasound Video. *IEEE Access* 2021; 9: 160249–160267.
33. Zhu F, Liu M, Wang F, Qiu D, Li R, Dai C. Automatic measurement of fetal femur length in ultrasound images: a comparison of random forest regression model and SegNet. *Math Biosci Eng* 2021; 18: 7790–7805.
34. Jang J, Park Y, Kim B, Lee SM, Kwon J-Y, Seo JK. Automatic Estimation of Fetal Abdominal Circumference From Ultrasound Images. *IEEE J Biomed Heal Informatics* 2018; 22: 1512–1520.
35. Kim B, Kim KC, Park Y, Kwon J-Y, Jang J, Seo JK. Machine-learning-based automatic identification of fetal abdominal circumference from ultrasound images. *Physiol Meas* 2018; 39: 105007.
36. Bano S, Dromey B, Vasconcelos F, Napolitano R, David AL, Peebles DM, Stoyanov D. AutoFB: Automating Fetal Biometry Estimation from Standard Ultrasound Planes, M Bruijne, P Cattin, S Cotin, N Padoy, S Speidel, Y Zheng, C Essert (eds). *Medical Image Computing and Computer Assisted Intervention - MICCAI 2021. Lecture Notes in Computer Science, Vol 12907. Springer: Cham, 2021; 228–238.*
37. Płotka S, Włodarczyk T, Klasa A, Lipa M, Sitek A, Trzciński T. FetalNet: Multi-task Deep Learning Framework for Fetal Ultrasound Biometric Measurements, T Mantoro, M Lee, MA Ayu, KW Wong, AN Hidayanto (eds). *Neural Information Processing, ICONIP 2021. Communications in Computer and Information Science, vol 1517. Springer: Cham, 2021; 257–265.*
38. Ghelich Oghli M, Shabanzadeh A, Moradi S, Sirjani N, Gerami R, Ghaderi P, Sanei Taheri M, Shiri I, Arabi H, Zaidi H. Automatic fetal biometry prediction using a novel deep convolutional network architecture. *Phys Medica* 2021; 88: 127–137.
39. Prieto JC, Shah H, Rosenbaum AJ, Jiang X, Musonda P, Price JT, Stringer EM, Vwalika B, Stamilio DM, Stringer JSA. An automated framework for image classification and segmentation of fetal ultrasound images for gestational age estimation. *Proc SPIE Int Soc Opt Eng* 2021; 11596.

40. Płotka S, Klasa A, Lisowska A, Seliga-Siwecka J, Lipa M, Trzciński T, Sitek A. Deep learning fetal ultrasound video model match human observers in biometric measurements. *Phys Med Biol* 2022; 67: 045013.
41. International Society of Ultrasound in Obstetrics and Gynecology; Bilardo CM, Chaoui R, Hyett JA, Kagan KO, Karim JN, Papageorghiou AT, Poon LC, Salomon LJ, Syngelaki A, Nicolaides KH. ISUOG Practice Guidelines (updated): performance of 11–14-week ultrasound scan. *Ultrasound Obstet Gynecol* 2023; 61: 127–143.
42. Ryou H, Yaqub M, Cavallaro A, Papageorghiou AT, Alison Noble J. Automated 3D ultrasound image analysis for first trimester assessment of fetal health. *Phys Med Biol* 2019; 64: 185010.
43. Cengiz S, Yaqub M. Automatic Fetal Gestational Age Estimation from First Trimester Scans, JA Noble, S Aylward, A Grimwood, Z Min, S-L Lee, Y Hu (eds). *Simplifying Medical Ultrasound, ASMUS 2021. Lecture Notes in Computer Science, vol 12967. Springer: Cham, 2021; 220–227. https://doi.org/10.1007/978-3-030-87583-1_22.*
44. Nie S, Yu J, Chen P, Wang Y, Zhang JQ. Automatic Detection of Standard Sagittal Plane in the First Trimester of Pregnancy Using 3-D Ultrasound Data. *Ultrasound Med Biol* 2017; 43: 286–300.
45. Kwitt R, Vasconcelos N, Razzaque S, Aylward S. Localizing target structures in ultrasound video – A phantom study. *Med Image Anal* 2013; 17: 712–722.
46. Burgos-Artizzu XP, Coronado-Gutiérrez D, Valenzuela-Alcaraz B, Bonet-Carne E, Eixarch E, Crispi F, Gratacós E. Evaluation of deep convolutional neural networks for automatic classification of common maternal fetal ultrasound planes. *Sci Rep* 2020; 10: 10200.
47. Baumgartner CF, Kamnitsas K, Matthew J, Fletcher TP, Smith S, Koch LM, Kainz B, Rueckert D. SonoNet: Real-Time Detection and Localisation of Fetal Standard Scan Planes in Freehand Ultrasound. *IEEE Trans Med Imaging* 2017; 36: 2204–2215.
48. Chen H, Wu L, Dou Q, Qin J, Li S, Cheng J-Z, Ni D, Heng P-A. Ultrasound Standard Plane Detection Using a Composite Neural Network Framework. *IEEE Trans Cybern* 2017; 47: 1576–1586.
49. Zhang B, Liu H, Luo H, Li K. Automatic quality assessment for 2D fetal sonographic standard plane based on multitask learning. *Medicine (Baltimore)* 2021; 100: e24427.
50. Yaqub M, Kelly B, Papageorghiou AT, Noble JA. A Deep Learning Solution for Automatic Fetal Neurosonographic Diagnostic Plane Verification Using Clinical Standard Constraints. *Ultrasound Med Biol* 2017; 43: 2925–2933.
51. Minaee S, Boykov Y, Porikli F, Plaza A, Kehtarnavaz N, Terzopoulos D. Image Segmentation Using Deep Learning: A Survey. *IEEE Trans Pattern Anal Mach Intell* 2022; 44: 3523–3542.
52. Salomon LJ, Alfirevic Z, Berghella V, Bilardo CM, Chalouhi GE, Da Silva Costa F, Hernandez-Andrade E, Malinger G, Munoz H, Paladini D, Prefumo F, Sotiriadis A, Toi A, Lee W. ISUOG Practice Guidelines (updated): performance of the routine mid-trimester fetal ultrasound scan. *Ultrasound Obstet Gynecol* 2022; 59: 840–856.
53. Malinger G, Paladini D, Haratz KK, Monteagudo A, Pilu GL, Timor-Tritsch IE. ISUOG Practice Guidelines (updated): sonographic examination of the fetal central nervous system. Part 1: performance of screening examination and indications for targeted neurosonography. *Ultrasound Obstet Gynecol* 2020; 56: 476–484.
54. Qu R, Xu G, Ding C, Jia W, Sun M. Standard Plane Identification in Fetal Brain Ultrasound Scans Using a Differential Convolutional Neural Network. *IEEE Access* 2020; 8: 83821–83830.
55. Cai Y, Droste R, Sharma H, Chatelain P, Drukker L, Papageorghiou AT, Noble JA. Spatio-temporal visual attention modelling of standard biometry plane-finding navigation. *Med Image Anal* 2020; 65: 101762.
56. Huang R, Xie W, Alison Noble J. VP-Nets : Efficient automatic localization of key brain structures in 3D fetal neurosonography. *Med Image Anal* 2018; 47: 127–139.
57. Wyburd MK, Jenkinson M, Namburete AIL. Cortical Plate Segmentation Using CNNs in 3D Fetal Ultrasound, B Papiież, A Namburete, M Yaqub, J Noble (eds). *Medical Image Understanding and Analysis MIUA 2020. Conference Proceedings. Communications in Computer and Information Science, Vol 1248. Springer: Cham, 2020; 56–68.*

58. Venturini L, Papageorgiou AT, Noble JA, Namburete AIL. Multi-task CNN for Structural Semantic Segmentation in 3D Fetal Brain Ultrasound, Y Zheng, B Williams, K Chen (eds). *Medical Image Understanding and Analysis, MIUA 2019. Conference Proceedings. Communications in Computer and Information Science, Vol 1065.* Springer: Cham; 2020: 164–173.
59. Hesse LS, Aliasi M, Moser F, Haak MC, Xie W, Jenkinson M, Namburete AIL. Subcortical segmentation of the fetal brain in 3D ultrasound using deep learning. *Neuroimage* 2022; 254: 119117.
60. Lin M, He X, Guo H, He M, Zhang L, Xian J, Lei T, Xu Q, Zheng J, Feng J, Hao C, Yang Y, Wang N, Xie H. Use of real-time artificial intelligence in detection of abnormal image patterns in standard sonographic reference planes in screening for fetal intracranial malformations. *Ultrasound Obstet Gynecol* 2022; 59: 304–316.
61. Patra A, Noble JA. Multi-anatomy localization in fetal echocardiography videos. In 2019 IEEE 16th International Symposium on Biomedical Imaging, 2019; 1761–1764.
62. Nurmaini S, Rachmatullah MN, Sapitri AI, Darmawahyuni A, Tutuko B, Firdaus F, Partan RU, Bernolian N. Deep Learning-Based Computer-Aided Fetal Echocardiography: Application to Heart Standard View Segmentation for Congenital Heart Defects Detection. *Sensors (Basel)* 2021; 21: 8007.
63. Dozen A, Komatsu M, Sakai A, Komatsu R, Shozu K, Machino H, Yasutomi S, Arakaki T, Asada K, Kaneko S, Matsuoka R, Aoki D, Sekizawa A, Hamamoto R. Image Segmentation of the Ventricular Septum in Fetal Cardiac Ultrasound Videos Based on Deep Learning Using Time-Series Information. *Biomolecules* 2020; 10: 1526.
64. Ramirez Zegarra R, Dall'Asta A, Ghi T. Mechanisms of Fetal Adaptation to Chronic Hypoxia following Placental Insufficiency: A Review. *Fetal Diagn Ther* 2022; 49: 279–292.
65. Sulas E, Ortu E, Raffo L, Urru M, Tumbarello R, Pani D. Automatic Recognition of Complete Atrioventricular Activity in Fetal Pulsed-Wave Doppler Signals. *Annu Int Conf IEEE Eng Med Biol Soc* 2018; 2018: 917–920.
66. Lakra PP, Kumar A, Mohanram N, Krishnamurthi G, Thittai AK. Deep-Learning based Identification of Frames Containing Foetal Gender Region During Early Second Trimester Ultrasound Scanning. 2019 IEEE International Ultrasonics Symposium (IUS) IEEE, 2019: 471–474.
67. GE Healthcare. SCANNAV™ Assist. <https://www.intelligentultrasound.com/scannav-assist/>.
68. Eggebø TM, Heien C, Økland I, Gjessing LK, Romundstad P, Salvesen KÅ. Ultrasound assessment of fetal head–perineum distance before induction of labor. *Ultrasound Obstet Gynecol* 2008; 32: 199–204.
69. Barbera AF, Pombar X, Perugino G, Lezotte DC, Hobbins JC. A new method to assess fetal head descent in labor with transperineal ultrasound. *Ultrasound Obstet Gynecol* 2009; 33: 313–319.
70. Chen P, Chen Y, Deng Y, Wang Y, He P, Lv X, Yu J. A preliminary study to quantitatively evaluate the development of maturation degree for fetal lung based on transfer learning deep model from ultrasound images. *Int J Comput Assist Radiol Surg* 2020; 15: 1407–1415.
71. Vaze S, Namburete AIL. Segmentation of Fetal Adipose Tissue Using Efficient CNNs for Portable Ultrasound, A Melbourne, R Licandro, M DiFranco, P Rota, M Gau, M Kampel, R Aughwane, P Moeskops, E Schwartz, E Robinson, A Makropoulos (eds). *Data Driven Treatment Response Assessment and Preterm, Perinatal, and Paediatric Image Analysis. PIPPI 2018, DATRA 2018. Lecture Notes in Computer Science, vol 11076.* Springer: Cham, 2018; 55–65.
72. Hermawati FA, Tjandrasa H, Suciati N. Phase-based thresholding schemes for segmentation of fetal thigh cross-sectional region in ultrasound images. *J King Saud Univ - Comput Inf Sci* 2022; 34: 4448–4460.
73. Dall'Asta A, Rizzo G, Masturzo B, Di Pasquo E, Schera GBL, Morganelli G, Ramirez Zegarra R, Maquina P, Mappa I, Parpinel G, Attini R, Roletti E, Menato G, Frusca T, Ghi T. Intrapartum sonographic assessment of the fetal head flexion in protracted active phase of labor and association with labor outcome: a multicenter, prospective study. *Am J Obstet Gynecol* 2021; 225: 171. e1–12.
74. Ghi T, Bellussi F, Eggebø T, Tondi F, Pacella G, Salsi G, Cariello L, Piastra A, Youssef A, Pilu G, Rizzo N. Sonographic assessment of fetal occiput position during the second stage of labor: how reliable is the transperineal approach? *J Matern Neonatal Med* 2015; 28: 1985–1988.

75. Ghi T, Eggebø T, Lees C, Kalache K, Rozenberg P, Youssef A, Salomon LJ, Tutschek B. ISUOG Practice Guidelines: intrapartum ultrasound. *Ultrasound Obstet Gynecol* 2018; 52: 128–139.
76. Ghi T, Conversano F, Ramirez Zegarra R, Pisani P, Dall'Asta A, Lanzone A, Lau W, Vimercati A, Iliescu DG, Mappa I, Rizzo G, Casciaro S, International Study group on Labor ANd Delivery Sonography (ISLANDS). Novel artificial intelligence approach for automatic differentiation of fetal occiput anterior and non-occiput anterior positions during labor. *Ultrasound Obstet Gynecol* 2022; 59: 93–99.
77. Ramirez Zegarra R, Dall'Asta A, Conversano F, Dr Trani MG, Morello R, Pisani P, Di Paola M, Casciaro S, Ghi T. Artificial Intelligence Algorithm for the automatic classification of anterior/posterior/transverse fetal occiput positions during labor. *Dreiländertreffen* 2022

التطورات في تقنيات التعلم العميق لتحسين تقييم التشوهات الجنينية في التصوير قبل الولادة: مراجعة التطبيقات الحالية والتوجهات المستقبلية

الملخص

الخلفية: أصبح التعلم العميق (DL) تقنية تحويلية في مجال التصوير الطبي، لا سيما في التقييمات قبل الولادة. تهدف تطبيقات خوارزميات التعلم العميق في التصوير الجنيني إلى معالجة التحديات مثل التحيز البشري والتفاوت بين الملاحظين، مع تحسين دقة التشخيص.

الطرق: تسلط هذه المراجعة الضوء على التطورات الحديثة في تطبيق تقنيات التعلم العميق لتقييم التشوهات الجنينية. تم إجراء بحث شامل في الأدبيات لجمع الأدلة حول فعالية التعلم العميق في مختلف جوانب التصوير قبل الولادة، بما في ذلك التقييم التشريحي، القياسات البيومترية، واكتشاف التشوهات الخلقية.

النتائج: تشير النتائج إلى أن نماذج التعلم العميق تقدم أداءً متفوقاً في تحديد التشريح الجنيني الطبيعي وغير الطبيعي مقارنة بالطرق التقليدية. وتُظهر هذه النماذج كفاءة عالية في تصنيف الصور، وتحديد مواقع الهياكل التشريحية، وتجزئة الميزات الرئيسية، مما يقلل بشكل كبير من أوقات الفحص ويحسن سير العمل. علاوة على ذلك، أظهرت العديد من الدراسات أن التعلم العميق يمكن أن يقلل من تأثير الخطأ البشري، محققاً تصنيفات تنافس أو تتجاوز تلك التي يقوم بها مختصو التصوير بالموجات فوق الصوتية ذوو الخبرة.

الاستنتاج: يحمل دمج تقنيات التعلم العميق في التصوير قبل الولادة وعداً كبيراً لتحسين القدرات التشخيصية وتحسين نتائج المرضى. ومع تطور هذه التقنيات، فإنها تقدم إمكانات لدعم الأطباء، لا سيما في المناطق ذات الموارد المحدودة حيث يكون الوصول إلى مختصين مهرة في الموجات فوق الصوتية محدوداً. يجب أن تركز الأبحاث المستقبلية على تحسين هذه النماذج وضمان قابليتها للتطبيق السريري لتعزيز فوائد التعلم العميق في رعاية التوليد.

الكلمات المفتاحية: التعلم العميق، التصوير الجنيني، التقييم قبل الولادة، التشوهات الخلقية، تكنولوجيا الموجات فوق الصوتية.